




# PRIMUSRS™

## SITE REQUIREMENT SPECIFICATIONS

Below is a layout of the recommended space requirement for the PrimusRS including the Patient Positioning Chair.

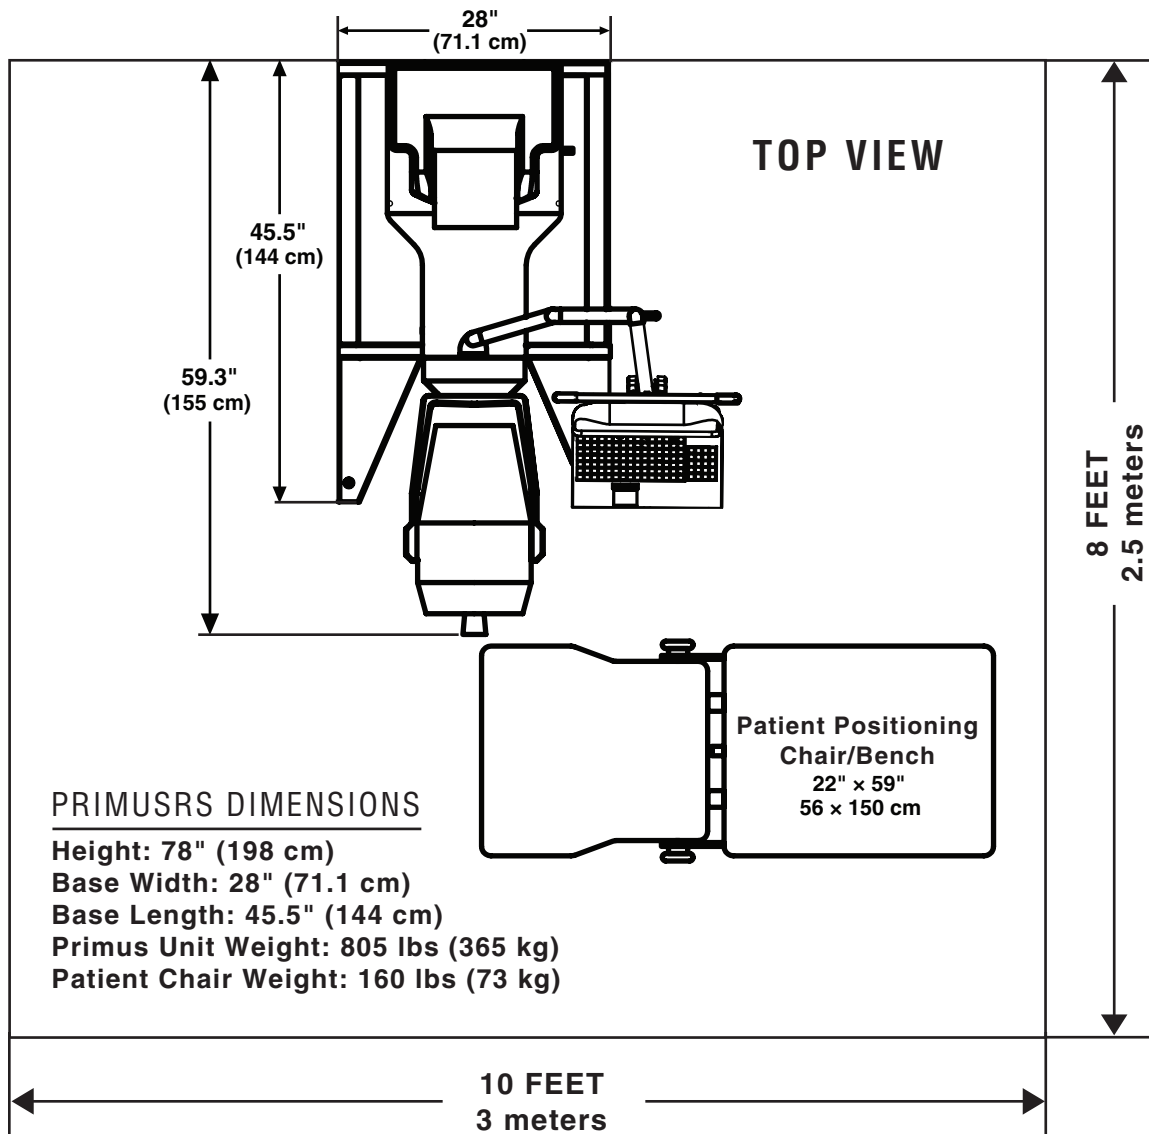

### ELECTRICAL REQUIREMENTS

**US/Canada: DEDICATED 110-125 volt circuit, 60 Hz, 20 amps**

**International: DEDICATED 220-240 volt circuit, 50 Hz, 10 amps**